

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument
State of Alaska

Serial #: 100380

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 06/28/2011

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.56: 0.079
LOT #: 34409080A1
EXPIRATION: 01/01/2012

BLANK TEST	0.000	14:27
INTERNAL STANDARD	VERIFIED	14:27
EXTERNAL STANDARD	0.079	14:28
BLANK TEST	0.000	14:29
EXTERNAL STANDARD	0.079	14:29
BLANK TEST	0.000	14:30
EXTERNAL STANDARD	0.079	14:30
BLANK TEST	0.000	14:31
EXTERNAL STANDARD	0.079	14:31
BLANK TEST	0.000	14:32
EXTERNAL STANDARD	0.079	14:32
BLANK TEST	0.000	14:33

Average = 0.0790
Std Dev = 0.0000

Diagnostic Check

VERSIONS

DMT: 1.02
PIC: 3.02
Modem: 2.0
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C	PASSED
Breath Tube = 44.8°C	PASSED

PUMP INFO

Flow Rate = 4.967 L/M	PASSED
-----------------------	--------

DETECTOR INFO

PUMP ON	PASSED
PUMP OFF	PASSED


FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD	PASSED
-------------------	--------


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

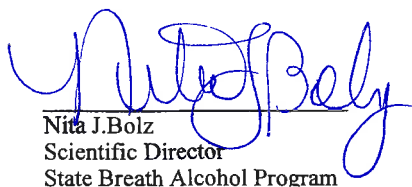
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

7/22/11

Subscribed and sworn before me this 22 day of July 20 11




Nikki Roth
Notary Public's Signature
My Commission Expires on with office


Nikki Roth
Notary Name


6/29/11